


Product Name :
Expansion Index Test Apparatus

Product Code :
NLAB-VOCATIONALTVET18025

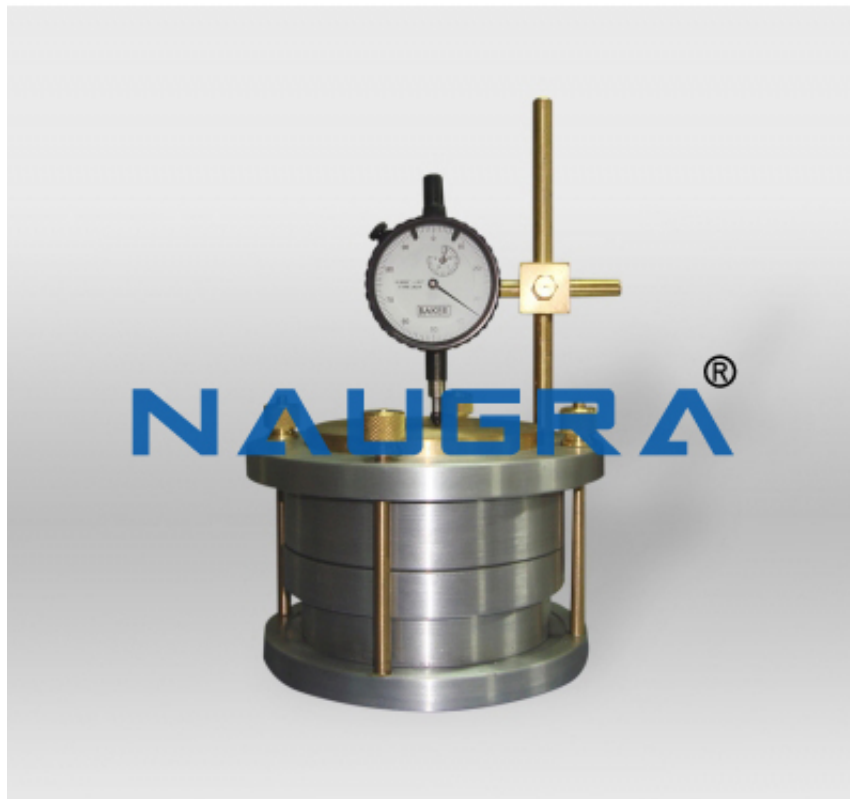

Description :

Expansion Index Test Apparatus

Technical Specification :

Construction: The unit consists of a cast aluminum base and collar, stainless steel specimen ring.

Base and Collar: Cast aluminum construction; brass hold-down rods.

Specimen Ring: Stainless steel; 101.6 x 25.4 mm (4" internal diam. x 1" h.).

Porous Stones: 101.4 x 12.7 mm (4" diam. x 1/2" thick).

Loading Weight: Brass; 5.7 kg (12.6 lbs.).

Dial Indicator: 0.3" range x 0.0001" graduations. 8 mm range x 0.002 mm graduations.

Test Duration: 24 hours or less on the cured sample

Naugralabequipments

Website: www.naugralabequipments.com, **Email:** sales@naugralabequipments.com

Address: 6148/6, Guru Nanak Marg, Ambala Cantt, Haryana, India. **Phone:** +91-9896600003